

Product Fitting Guide

Succeed Succeed Ws

For more information please contact: Luzerne Optical Laboratories, Ltd. 1-800-233-9637 or at www.LuzerneOptical.com

SEIKO INTERNAL FREE-FORM PROGRESSIVE LENSES WITH PATENTED 100% BACK SURFACE TECHNOLOGY

Measure Patient PD & Select Frame

- Use a pupilometer to obtain an accurate monocular PD. Choose a lightweight, well-proportioned frame, with adjustable nose pads.

Adjust Frame

- Fit the frame as close to the face as possible without touching skin or eyelashes. The pupil should be located in the upper half of the frame, between 50 and 75% of the total frame height.
- Set the pantoscopic tilt to approximately 10°. Decrease the tilt if the distance PD is below 58mm. Increase tilt if distance PD exceeds 68mm.

Measure Fitting Height & Confirm PD

- Have the patient wear the frame for a few minutes to adjust to it. Then, with the patient looking straight ahead, place a small dot on the sample lens at the center of each pupil. Draw a horizontal line through each dot. Double-check to make sure the lines bisect the pupils.

- Place the frame on the fitting guide scale (reverse) so that the vertical line labeled "O" divides the bridge in half, and the dots and lines on the sample lenses line up on the horizontal line.
- Confirm the PD using the scale. Measure the fitting height from the lines on the sample lenses to the deepest part of the frame.

**Note: Follow fitting height recommendations.
Do not fit below minimum heights.**

Verify Cutout

- Place the frame over the cutout circle on the fitting guide, and align the pupil dot and horizontal line that you made on the sample lens with the fitting cross. If the frame does not fit within the circle, the lens may not cut out correctly.

Verify Fitting Height and PD

- When the lab returns your lenses, they should have verification markings. If not, place the lenses face down on the chart to draw the markings.

- Confirm the fitting height and monocular PD by placing the frame face down on the fitting guide so that the vertical line labeled "O" divides the bridge in half, and the fitting cross on the lenses rest on the horizontal line.
- Place the frame on the patient and verify that the fitting cross is at the pupil center. Adjust the nose pads if necessary.
- On final fitting, check tilt and adjust if necessary until the best fit is achieved (for optimal distance and reading vision). These lenses are designed so that the pupil sits right at the beginning of the intermediate corridor. In the rare case where the patient experiences visual difficulty at the pupil location, lowering the frame slightly (1-2mm) may increase wearing comfort.

Instruct the Patient on Proper Use

- Use the reading card included on the certificate of authenticity to demonstrate the use of distance, intermediate and near zones.

SEIKO
SEIKO Optical Products of America, Inc.

Transitions® VI
ADVANCED PERFORMANCE
FOR HEALTHY SIGHT

Transitions and the swirl are registered trademarks of Transitions Optical, Inc.

Seiko Epson Corporation owns the intellectual property rights (patent #6,019,470) in the United States, to produce/distribute/sell/market lenses that combine the toric and progressive powers onto the back surface (eye side) of the lens.






SEIKO

Succeed Succeed Ws

SEIKO INTERNAL FREE-FORM PROGRESSIVE LENSES WITH PATENTED 100% BACK SURFACE TECHNOLOGY

Lens	Min. Fit. Height	Corridor Length
Succeed WS	15mm 17mm	11mm 13mm
Succeed	17mm 19mm	13mm 15mm

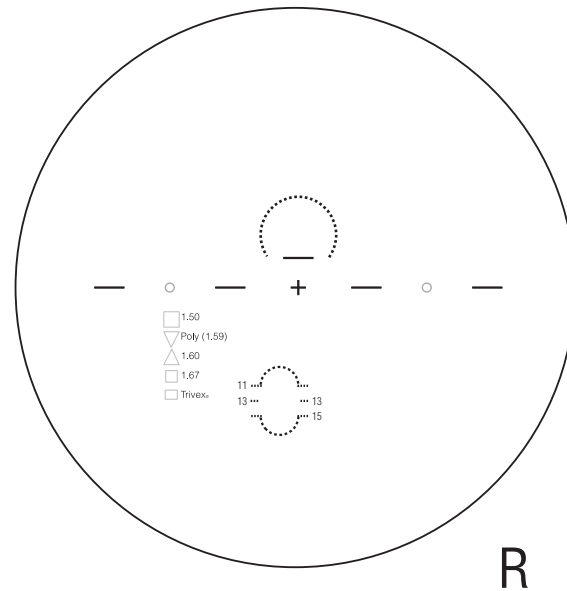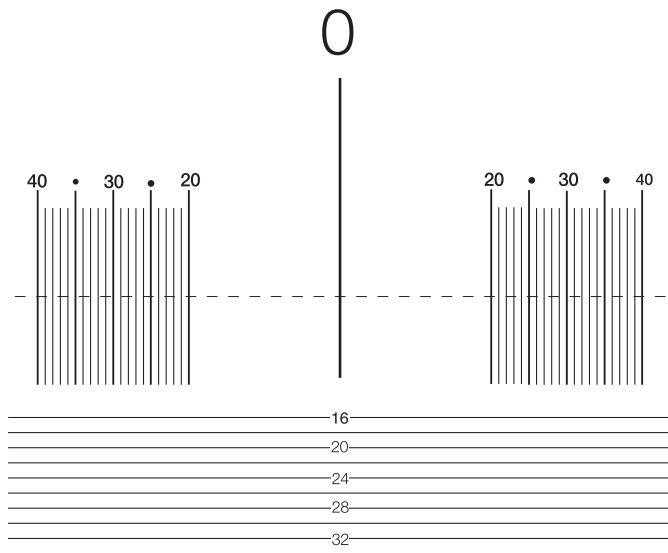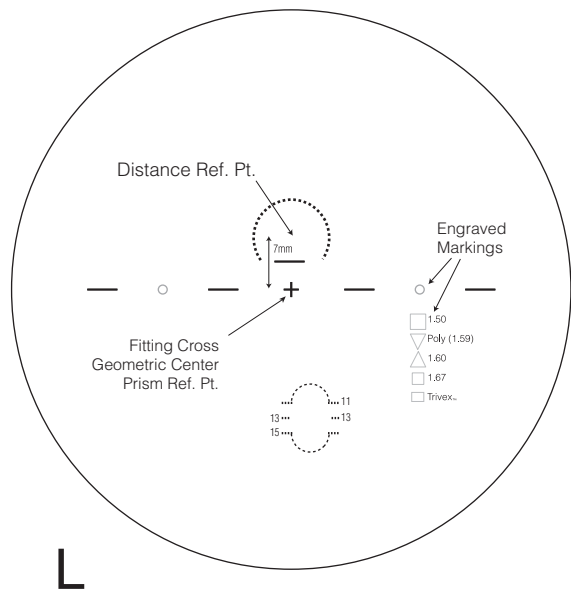

For more information please contact: Luzerne Optical Laboratories, Ltd. 1-800-233-9637 or at www.LuzerneOptical.com